

Motorized Retractable Monitor

LS19A

User Manual



Read this instructions carefully before using the device



warning

In order to make sure the device is working properly, please follow below instructions:

a. If found any abnormal situation, please cut off the power, pull off the plug and contact your supplier. To avoid any fire accident, DON'T use device in following situations:

- If you found peculiar smell or fog comes from inside of unit.
- If have water or metal parts going to the unit.
- If the lift unit box is broken.
- If the wire is broken inside.

b. As the device is high pressure inside, please DON'T open the unit box at random to avoid fire or electric shock,.

c. DON'T put any conducting liquid on top of the device, to avoid electric shock or fire.

d. The device is I type; the power should be connected to ground.

e. The device is suitable for AC 220V 50Hz.

1. Operation instructions

1.1 packing list

NO.	description	remark
1	Monitor lift	1set
2	Power plug	1pcs
3	RS-485 cable	1pcs

4	User manual	1set
---	-------------	------

1.2 Interface on the bottom case (from left to right)



- HDMI in
- DVI in (optional)
- VGA in (optional)
- USB input, up: USB data, down: USB touch
- RS485 in (1: RS-485 +, 2: RS-485 -, 5: GND)
- RS485 out (use for cluster control)
- ANT Remote control (optional)
- Spare: PC SW power on; SA SW signal switch
- AC 220V input power socket

1.3 Control Introduction:

RS485 Software Control: 9 holes interface with the computer serial port. 232/485 intermediate bridge converter.



connector(female)



connector(male)

Top panel button:



Control Button: (The Red indicator light is power indicator, if it is red, mean no signal, green is with signal)

Icon	Button
	Stop
	Up
	Down
	Tilting
	Tilting

1.4 Introduction to Manipulation

Display button :



- LED: indicated light, NO SIGNAL: the light is red,
WITH SIGNAL: Light is green.
-  : display power on/off
-  : Variable Button (-)
-  : Variable Button (+)
- AUTO: Automatic adjustment button and have

return function.


- MENU

2. Characteristics and main parameters


2.1 Structural and functional characteristics

AX-19F motorized monitor lift is using the synchronous belt pulley with a straight line for rising and falling, the tilt driver will as an individual part and the max. angle is 0~20°adjustable. Stable structure and low noise, using the aluminum frame match with the toughened glass, more elegant. The product uses the desktop embedded design, could hide in the table perfectly.

2.2 Cut out size

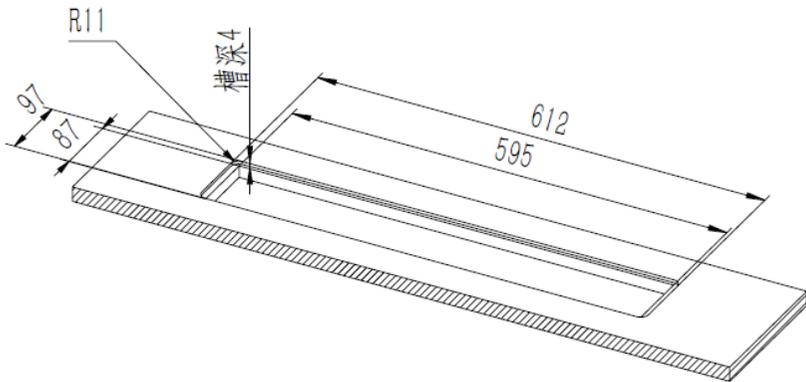

2.3 product size

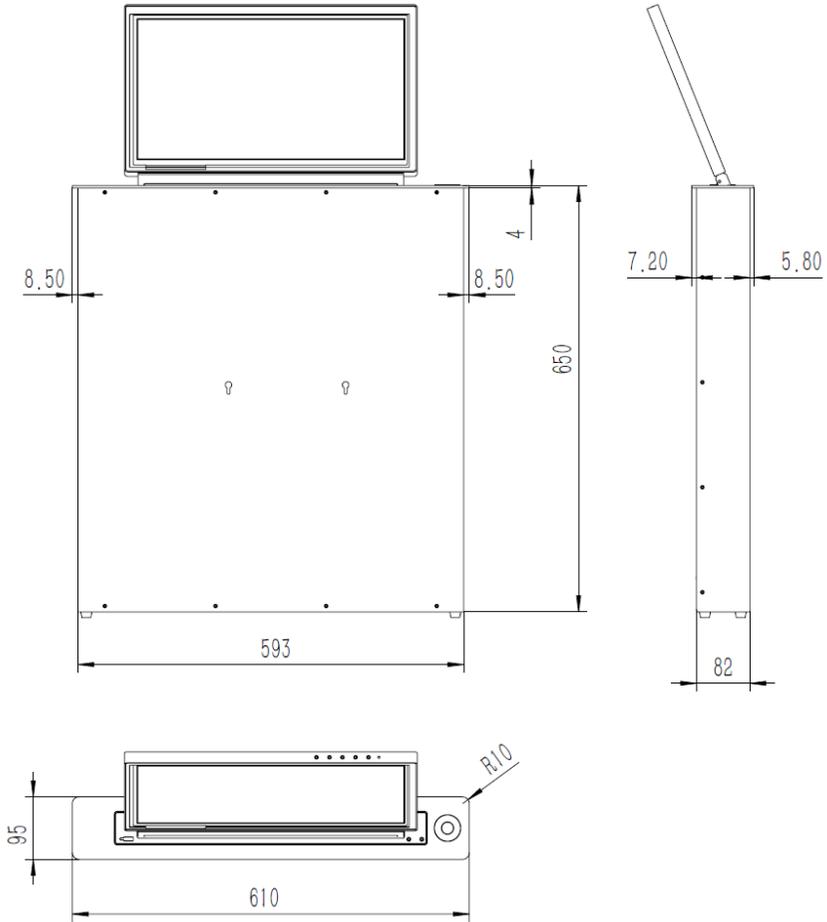

2.4 Technical parameters of lifts

No.	Item	Data
1	Voltage	AC 220V 50HZ
2	Power consumption	<50W
3	Single running time	13S
4	Tilting	0-20° motorized adjustable

2.5 Technical parameters of display screen

NO.	Item	Data
1	Screen size	18.4 inch
2	Screen type	LVDS
3	Resolution	1920*1080
4	Aspect ratio	16:9
5	Contrast ratio	800:1
6	Brightness	300 cd/m ²
7	Signal type	VGA/HDMI (automatically)
8	View angle	85/85/85/85

3. Installation instructions

- Please remove 4 pcs safety screws & remove the foam inside the case before charging (the screws are in the, back, right & left side of cover plate)

- Put the lift into to table cutting hole, and flushing the panel with the table.



- Connect the video signal cable (VGA or HDMI).
- Connect the USB touch line, otherwise the touch screen will not work
- For central control, please connect the RS485.
- Connect the power, when the light is bright, push the button of “up/fall back” to finish the Automatic elevation process. After that, you could push “up/down” button to adjust the angle as you want.

4. Central control code

All up	FF AC E1 FF 00 00 DD 01 DC
Stop	FF AC E1 FF 00 00 CD 01 CC
All down	FF AC E1 FF 00 00 ED 01 EC


5. Computer App control

- If required, please contact us for RS485 control software “Multifunctional-Lift Control Center V2.0 _win”。
- Prepare a converter of RS232 to RS485 or USB to RS485, and install the driver, connect all the lift which need to be control
- Download and install the software in English version, log in as admin with pass word 88888888, please adjust the langue and the correct COM after access in.
- Operate the assembly according to the app instruction

6. FAQ and Solutions

No.	Fault phenomenon	Reason
1	NO display	Check the power on or off? Check the signal, is it interrupted?
2	Character ambiguity	Does it match with the computer resolution? Is it the contrast and brightness adjustment correct?
3	Black screen	It would turn off the brightness automatically without signal, Is brightness adjustment minimum? Long press of the "Auto" key may cause shutdown and the indicator to turn red.
4	Invalid touch function	Make sure the USB connection is correct or connect well
5	The indicator is not on	Check if the fuse is damaged. If it is damaged, replace the fuse

		with 3.15A specification.
--	--	---------------------------



Safety Pipe Location of National Standard Socket

- Subject to change without prior notice, the current production model shall prevail.
- For any enquiry, please contact our service center.